



CODEN [USA]: IAJ PBB

ISSN : 2349-7750

INDO AMERICAN JOURNAL OF
PHARMACEUTICAL SCIENCES

SJIF Impact Factor: 7.187

<https://doi.org/10.5281/zenodo.21360770>Available online at: <http://www.iajps.com>

Research Article

**ANALYTICAL METHOD AND VALIDATION FOR
QUALITATIVE DETERMINATION OF ETELCA CETIDE IN
BULK FORM AND MARKETED PHARMACEUTICAL
PREPARATION****Dr. Khaja Zeeyauddin^{*1}, Katravath Divya², Kothagolla Krishna², Erani Nikith²,
Gangapuram Manikanta Goud²**1- Professor, Department Of Pharmacology, Aiops, Avanthi Institute of Pharmaceutical
Sciences, Hayathnagar, Gunthapally, Hyderabad, Telangana-5015122-Students, Department Of Pharmaceutical Analysis, Avanthi Institute of Pharmaceutical
Sciences, Hayathnagar, Gunthapally, Hyderabad, Telangana-501512**Abstract:****Objective:** The current investigation was pointed at developing and progressively validating novel, simple, responsive and stable RP-HPLC method for the Quantitative Determination of Etelcalcetide in active pharmaceutical ingredient and Marketed Pharmaceutical Dosage form.**Methods:** A simple, selective, validated and well-defined stability that shows isocratic RP-HPLC methodology for the quantitative determination of Etelcalcetide. The chromatographic strategy utilized Symmetry C18, 250 mm x 4.6 mm i.d. 5µm particle size, using isocratic elution with a mobile phase consists of Methanol and Phosphate Buffer (0.02M) (pH-3.8) was taken in the ratio of 70: 30% v/v. A flow rate of 1.0 ml/min and a detector wavelength of 245nm utilizing the UV detector were given in the instrumental settings. Validation of the proposed method was carried out according to an international conference on harmonization (ICH) guidelines.**Results:** LOD and LOQ for the active ingredients were established with respect to test concentration. The calibration charts plotted were linear with a regression coefficient of $R^2 > 0.999$, means the linearity was within the limit. Recovery, specificity, linearity, accuracy, robustness, ruggedness were determined as a part of method validation and the results were found to be within the acceptable range.**Conclusion:** The proposed method to be fast, simple, feasible and affordable in assay condition. During stability tests, it can be used for routine analysis of the selected drugs.**Key Words:** Etelcalcetide, RP-HPLC, Method Development, Validation, Accuracy, Precision.**Corresponding author:****Dr. Khaja Zeeyauddin,**
Professor, Department Of Pharmacology,
Aiops, Avanthi Institute of Pharmaceutical Sciences,
Hayathnagar, Gunthapally,
Hyderabad, Telangana-501512

Please cite this article in press **Khaja Zeeyauddin et al., Analytical Method And Validation For Qualitative Determination Of Etelcalcetide In Bulk Form And Marketed Pharmaceutical Preparation., Indo Am. J. P. Sci, 2026; 13(07).**

INTRODUCTION:

Etelcalcetide is a calcium sensing receptor agonist used to treat secondary hyperparathyroidism in patients with chronic kidney disease who require hemodialysis¹. Etelcalcetide is a Calcimimetic drug for the treatment of secondary hyperparathyroidism in patients undergoing hemodialysis. Etelcalcetide was approved (trade name Parsabiv) for the treatment of secondary hyperparathyroidism (HPT) in adult patients with chronic kidney disease (CKD) on hemodialysis in February, 2017. Following a single intravenous bolus administration of Etelcalcetide, PTH levels

decreased within 30 minutes post dose². In the single-dose study, the extent and duration of the reduction in PTH increased with increasing dose. Reduction in PTH levels correlated with plasma Etelcalcetide concentrations in hemodialysis patients. The reduction in PTH resulted in reductions in calcium and attenuation of post-dialytic phosphate elevation. The effect of reducing PTH levels was maintained throughout the 6-month dosing period when Etelcalcetide was administered by intravenous bolus three times a week³. The Chemical Structure of Etelcalcetide is shown in following figure-1.

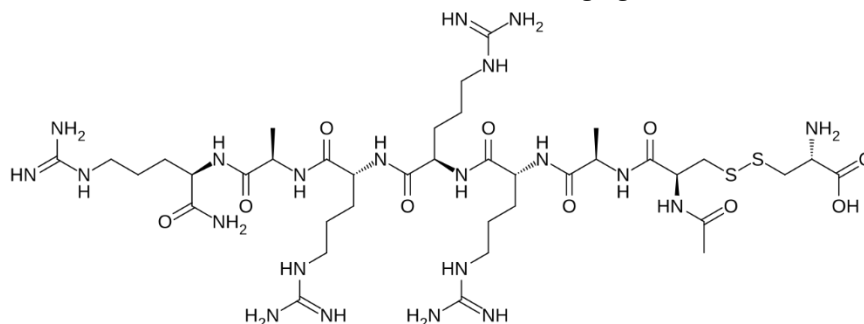


Fig-1: Chemical Structure of Etelcalcetide

EXPERIMENTAL**Materials and Instruments:**

The following are the list of instruments/Equipments, chemicals/reagents and standards to perform the HPLC Analysis of the drug Etelcalcetide.

Equipments:

Table-1: List of Equipments

S.No.	Instruments/Equipments/Apparatus
1.	HPLC WATERS with Empower2 Software with Isocratic with UV-Visible Detector.
2.	T60-LABINDIA UV – Vis spectrophotometer
3.	High Precision Electronic Balance
4.	Ultra Sonicator (Wensar wuc-2L)
5.	Thermal Oven
6.	Symmetry C ₁₈ Column, 250 mm x 4.6 mm and 5µm particle size
7.	P ^H Analyser (ELICO)
8.	Vaccum Filtration Kit (Labindia)

Chemicals and Reagents:

Table-2: List of Chemicals used

S.No.	Name	Grade	Manufacturer/Supplier
1.	HPLC grade water	HPLC	Sd fine-Chem ltd; Mumbai
2.	Methanol	HPLC	Loba Chem; Mumbai.
3.	Ethanol	A.R.	Sd fine-Chem ltd; Mumbai
4.	Acetonitrile	HPLC	Loba Chem; Mumbai.
5.	DMSO	A.R.	Sd fine-Chem ltd; Mumbai
6.	DMF	A.R.	Sd fine-Chem ltd; Mumbai

Working Standard: Working Standard of Etelcalcetide: 10ppm

HPLC Instrumentation & Conditions: The HPLC system employed was **HPLC WATERS** with Empower2 Software with Isocratic with UV-Visible Detector⁴.

Standard Preparation for UV-Spectrophotometer Analysis:

The Standard Stock Solutions – 10 mg of Etelcalcetide standard was transferred into 10 ml volumetric flask, dissolved & make up to volume

with Methanol. Further dilutions were done by transferring 1 ml of the above solution into a 10ml volumetric flask and make up to volume with methanol to get 10ppm concentration⁵.

It scanned in the UV spectrum in the range of 200 to 400nm. This has been performed to know the maxima of Etelcalcetide, so that the same wave number can be utilized in HPLC UV detector for estimating the Etelcalcetide.

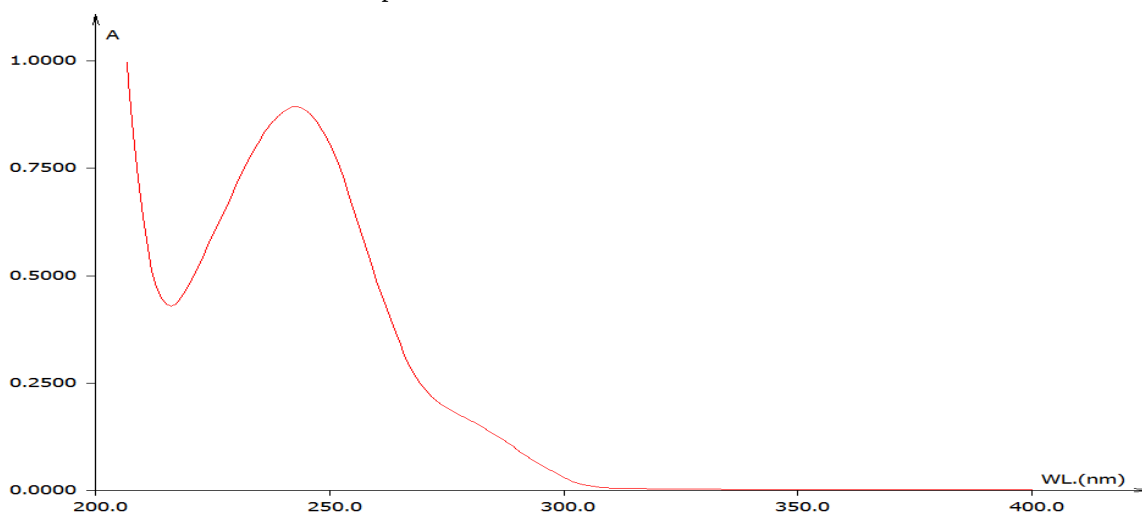


Fig-2: UV-Spectrum for Etelcalcetide

Observation: While scanning the Etelcalcetide solution we observed the maxima at 245nm.

DIFFERENT TRIALS FOR CHROMATOGRAPHIC CONDITIONS

Table-3: Different Chromatographic Conditions

Column Used	Mobile Phase	Flow Rate	Wave length	Observation	Result
Zorbax C ₁₈ , 250 mm x 4.6 mm and 5µm Column	Methanol : Acetonitrile = 30 : 70	0.9 ml/min	245nm	Extra peaks	Method rejected
Phenomenex C ₁₈ , 250 mm x 4.6 mm and 5µm Column	Methanol : Acetonitrile = 60 : 40	1.0 ml/min	245nm	Stabilization was not Good	Method rejected
Symmetry C ₁₈ , 250 mm x 4.6 mm and 5µm Column	Methanol : Acetonitrile = 50 : 50	1.0 ml/min	245nm	Improper peak separation	Method rejected
Symmetry C ₁₈ , 250 mm x 4.6 mm and 5µm Column	Methanol : Phosphate Buffer (0.01M) (pH-2.8) = 40 : 60	1.0 ml/min	245nm	Tailing peaks	Method rejected
Symmetry C ₁₈ , 250 mm x 4.6 mm and 5µm Column	Methanol : Phosphate Buffer (0.02M) (pH-3.2) = 60 : 40	1.0 ml/min	245nm	Tailing peaks	Method rejected
Symmetry C ₁₈ , 250 mm x 4.6 mm and 5µm Column	Methanol : Phosphate Buffer (0.02M) (pH-3.8) = 70 : 30	1.0 ml/min	245nm	Proper Peak	Method Accepted

Preparation of 0.02M Phosphate Buffer (pH-3.8): Prepare 800 mL of distilled water in a suitable container. Add 2.72172g of Potassium dihydrogen Phosphate to the solution to the solution. Adjust solution to final desired pH 3.8 using diluted solution of orthophosphoric acid and add distilled water until volume is 1 Litre⁶.

Preparation of Mobile Phase: Mix a mixture of 0.02M Phosphate Buffer (pH-3.8) 700 ml (70%) and 300 ml Methanol HPLC (30%) and degas in ultrasonic water bath for 15 minutes. Filter through 4.5 µ filter under vacuum filtration.

Optimized Chromatographic Conditions:

Column : Symmetry C18, 250 mm x 4.6 mm i.d.5µm particle size
 Mobile Phase : Methanol: Phosphate Buffer (0.02M) (pH-3.8) (70: 30% v/v)
 Flow Rate : 1.0ml/minute
 Wave length : 245 nm
 Injection volume : 10 µl
 Run time : 7 minutes
 Column temperature : Ambient

Preparation of Standard Solution:

Accurately weigh and transfer 10 mg of Etelcalcetide working standard into a 10ml of clean dry volumetric flasks add about 7ml of Diluents and sonicate to dissolve it completely and make volume up to the mark with the same solvent. (Stock solution)

Further pipette out 0.1ml of Etelcalcetide from the above stock solutions into a 10ml volumetric flask and dilute up to the mark with Diluent.

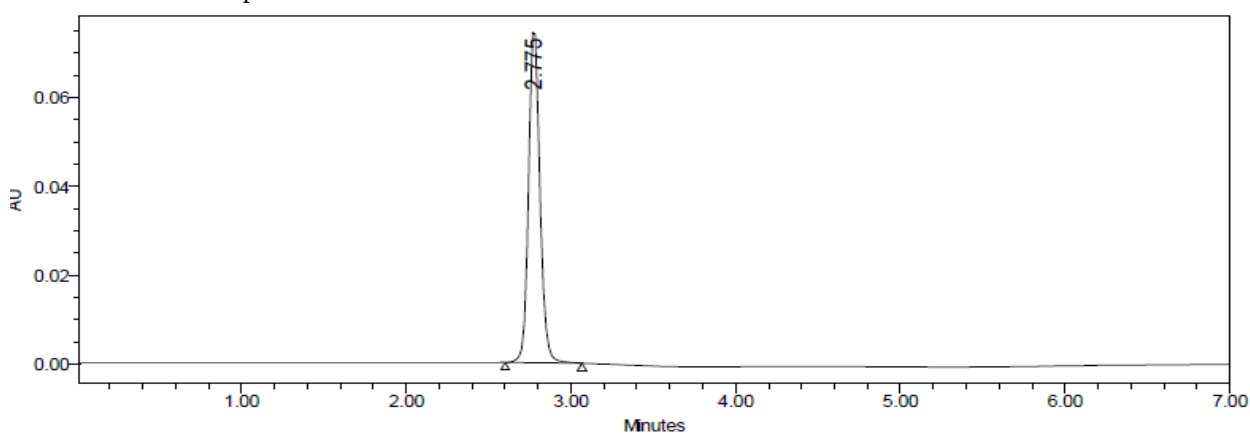


Fig-3: Optimized Chromatogram for Etelcalcetide

Observation: The selected and optimized mobile phase was Methanol: Phosphate Buffer (70: 30% v/v) and conditions optimized were flow rate (1.0 ml/minute), wavelength (245nm), Run time was 07 mins. Here the peak has shown better theoretical plate count and symmetry. The proposed chromatographic conditions were found appropriate for the quantitative determination of the Etelcalcetide drug⁷⁻¹⁰.

Method Validation:

System Suitability Test

System suitability testing is an integral part of many analytical procedures. The tests are based on the concept that the equipment, electronics, analytical operations and samples to be analysed constitute an integral system that can be evaluated as such. Following system suitability test parameters were established¹¹⁻¹³. The data are shown in Table-4 & 5.

Table-4: Data of System Suitability Test

S.No.	Injection No.	RT	Area	Height	USP Plate Count	USP Tailing
1	Injection 1	2.786	715268	47844	5857	1.36
2	Injection 2	2.784	716584	46985	5986	1.38
3	Injection 3	2.768	715364	47258	5784	1.35
4	Injection 4	2.789	714895	47152	5896	1.34
5	Injection 5	2.784	716587	47258	5749	1.36
6	Injection 6	2.781	718549	47985	5657	1.39
Mean			716207.8		5821.5	1.36
S.D			1347.976			
%RSD			0.18821			

Table-5: Acceptance Criteria and Result

S.No.	Parameter	Limit	Result
1	Tailing factor	$T \leq 2$	1.36
2	Theoretical plate	$N > 2000$	5821.5

Accuracy:

Recovery Study: To determine the accuracy of the proposed method, recovery studies were carried out by adding different amounts (80%, 100%, and 120%) of pure drug of Etelcalcetide were taken and 3 replications of each has been injected to HPLC system¹⁴. From that percentage recovery values were calculated from the linearity equation $y = 74143x + 7294.9$. The results were shown in table-6.

Table-6: Accuracy Readings

Sample ID	Concentration ($\mu\text{g/ml}$)		Peak Area	% Recovery of Pure drug	Mean % Recovery	% Mean Recovery = 100.364%
	Amount Injected	Amount Recovered				
S ₁ : 80 %	8	8.013	601425	100.162	Mean = 100.195%	
S ₂ : 80 %	8	8.012	601396	100.150		
S ₃ : 80 %	8	8.022	602123	100.275		
S ₄ : 100 %	10	10.038	751584	100.380	Mean = 100.356	
S ₅ : 100 %	10	10.039	751642	100.390		
S ₆ : 100 %	10	10.030	750969	100.300		
S ₇ : 120 %	12	12.057	901253	100.475	Mean = 100.541	
S ₈ : 120 %	12	12.073	902431	100.608		
S ₉ : 120 %	12	12.065	901864	100.541		

Observation: From the Accuracy Method, we observed that the mean %Recovery of the drug is 99.686 which are within the range of 98-102%.

Precision:**Repeatability**

The precision of each method was ascertained separately from the peak areas & retention times obtained by actual determination of six replicates of a fixed amount of drug Etelcalcetide (API). The percent relative standard deviation was calculated for Etelcalcetide¹⁵⁻¹⁷.

Table-7: Results of Repeatability readings

HPLC Injection Replicates of Etelcalcetide	Retention Time	Peak Area	Theoretical Plates	Tailing Factor
Replicate – 1	2.777	716984	5986	1.36
Replicate – 2	2.795	715698	5897	1.37
Replicate – 3	2.789	716859	5869	1.39
Replicate – 4	2.797	718548	5967	1.37
Replicate – 5	2.797	714895	5984	1.35
Replicate – 6	2.799	715986	5879	1.38
Average		716495	5930.333	1.37
Standard Deviation		1268.126		
% RSD		0.17699		

Observation: From the Precision method, we observed that the %RSD of the Peak Area is 0.176 which are within the acceptable range as per ICH guidelines.

Intermediate Precision:

The Intermediate Precision consists of two methods¹⁸:-

Intra Day: In Intra Day process, the 80%, 100% and 120% concentration are injected at different intervals of time in same day.

Inter Day: In Inter Day process, the 80%, 100% and 120% concentration are injected at same intervals of time in different days.

Table-8: Peak results for Intra-Day Precision

S.No.	Name	RT	Area	Height	USP Tailing	USP Plate Count	Injection
1	Etelcalcetide	2.784	716587	48685	1.38	5954	1
2	Etelcalcetide	2.768	717845	48698	1.39	5935	2
3	Etelcalcetide	2.786	716857	46989	1.36	5798	3
4	Average		717096.3	48124	1.376	5895.66	
5	S.D		662.2698				
6	% RSD		0.092354				

Table-9: Peak results for Inter-Day Precision

S.No.	Name	RT	Area	Height	USP Tailing	USP Plate Count	Injection
1	Etelcalcetide	2.780	716987	49867	1.34	5968	1
2	Etelcalcetide	2.794	718695	48574	1.33	5998	2
3	Etelcalcetide	2.775	718542	48569	1.39	5859	3
4	Average		718074.7	49003.33	1.353333	5941.667	
5	S.D		945.0483				
6	% RSD		0.131609				


Observations: The intra & inter day variation of the method was carried out for standard deviation & % RSD (% RSD < 2%) within a day & day to day variations for Etelcalcetide revealed that the proposed method is precise.

Linearity & Range:

To evaluate the linearity, serial dilution of analyte were prepared from the stock solution was diluted with mobile phase to get a series of concentration ranging from 6-14µg/ml. The prepared solutions were sonicated. From these solutions, 10µl injections of each concentration were injected into the HPLC system and chromatographed under the optimized conditions¹⁹⁻²². Calibration curve was constructed by plotting the mean peak area (Y-axis) against the concentration (X-axis).



Table-10: Linearity Concentrations of Etelcalcetide

S.No.	Concentration (in ppm)	Peak Area
1	0	0
2	6	457896
3	8	607574
4	10	752268
5	12	896587
6	14	1036579

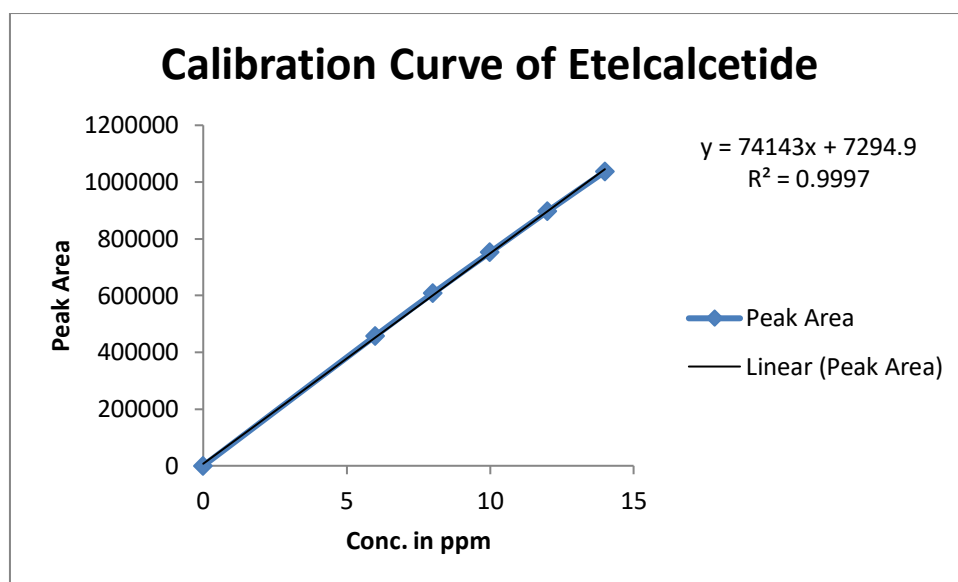**Fig-4: Calibration Curve of Etelcalcetide**

Observation: We observed that the calibration curve showed good linearity in the range of 6-14 $\mu\text{g/ml}$, for Etelcalcetide with correlation coefficient (R^2) of 0.9997. A typical calibration curve has the regression equation of $y = 74143x + 7294.9$ for Etelcalcetide.

Specificity: Specificity of the pharmaceutical analysis is the ability to measure accurately and specifically the concentration of API, without interference from other active ingredients, diluents, mobile phase. Solutions of mobile phase, sample solution, standard solution were injected into liquid chromatography. Retention times of samples and standard were compared²³.

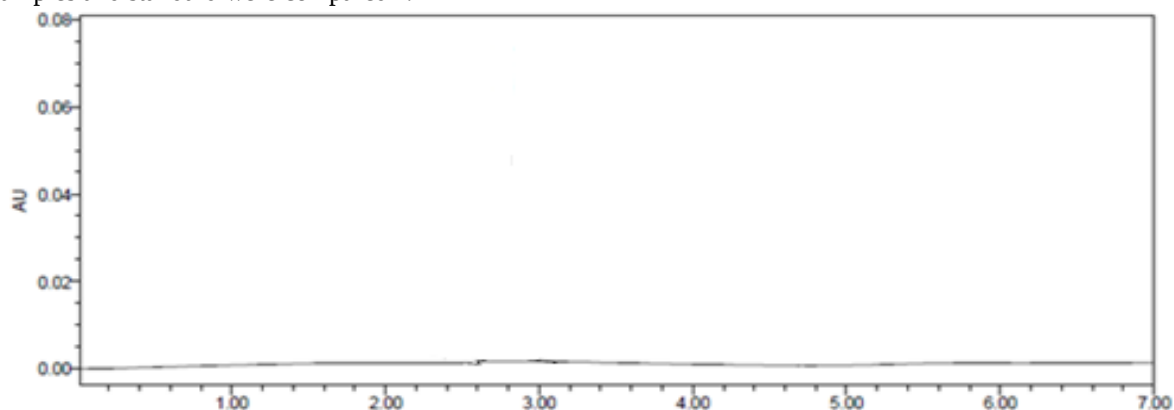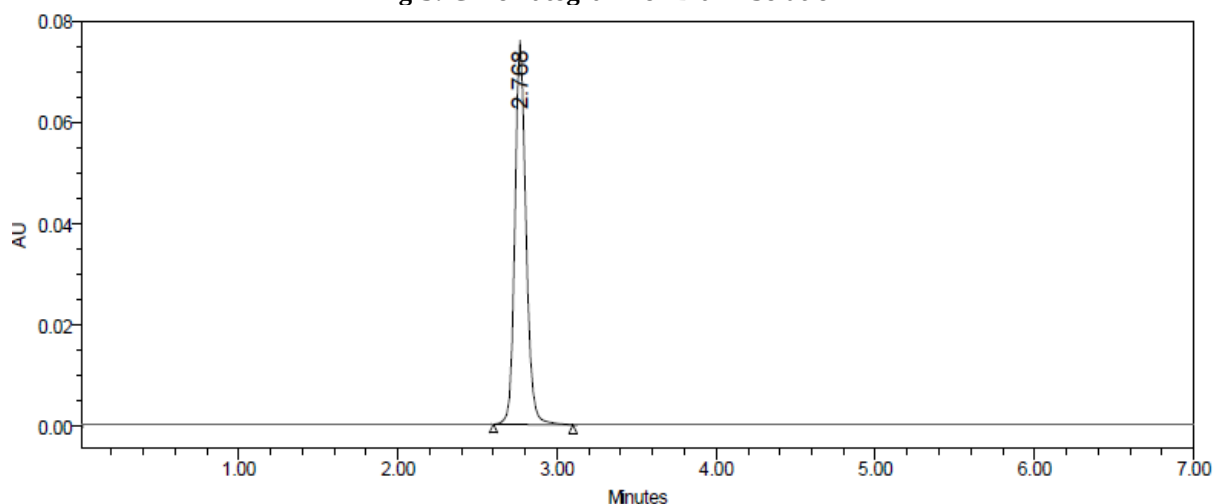**Fig-5: Chromatogram for Blank Solution****Fig-6: Optimized Chromatogram for Etelcalcetide Standard**

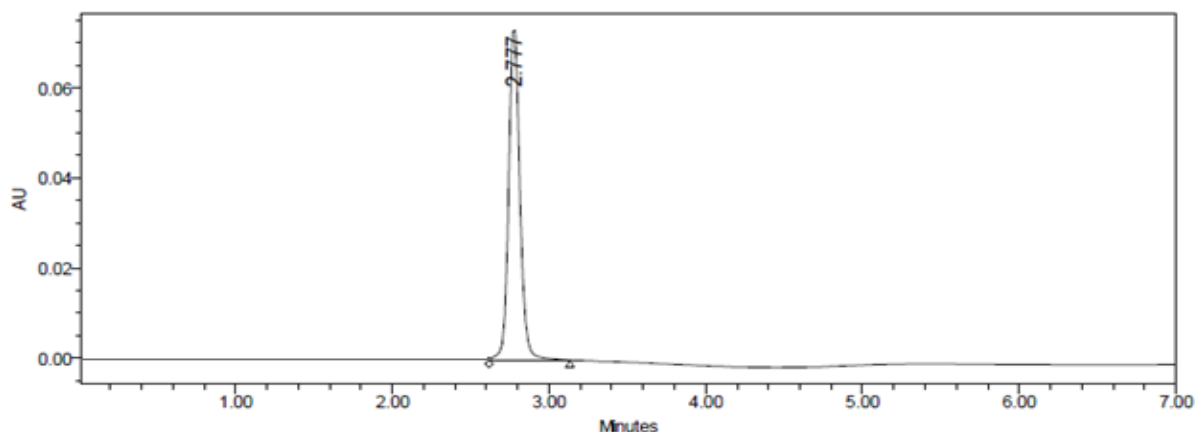


Fig-7: Optimized Chromatogram for Etelcalcetide Sample

Method Robustness: Influence of small changes in chromatographic conditions such as change in flow rate 1ml (± 0.1 ml/min), Wavelength of detection 245nm (± 2 nm) & organic phase content in mobile phase 60 (± 5 %) studied to determine the robustness of the method are also in favour of (Table-, % RSD <2%) the developed RP-HPLC method for the analysis of Etelcalcetide (API)²⁴⁻²⁵.

Table-11: Results of Method Robustness Test

Change in Parameter	Theoretical Plates	Tailing Factors
Flow (1.1 ml/min)	5954	1.35
Flow (0.8 ml/min)	6188	1.39
More Organic (70+5)	5748	1.41
Less Organic (70-5)	6185	1.48
Wavelength of Detection (250 nm)	6184	1.69
Wavelength of detection (240nm)	6247	1.47
Temperature (30 °C)	6324	1.34
Temperature (20 °C)	6985	1.32

LOD & LOQ: The detection limit (LOD) and quantization limit (LOQ) may be expressed as:

$$\text{L.O.D.} = 3.3(\text{SD}/S).$$

$$\text{L.O.Q.} = 10(\text{SD}/S)$$

Where, SD = Standard deviation of the response

S = Slope of the calibration curve

The slope S may be estimated from the calibration curve of the analyte.

The Minimum concentration level at which the analyte can be reliably detected (LOD) & quantified (LOQ) were found to be 0.507 & 1.539 $\mu\text{g/ml}$ respectively²⁶⁻²⁷.

Estimation of Etelcalcetide in Pharmaceutical Dosage Form

Twenty tablets were taken and the I.P. method was followed to determine the average weight. Above weighed tablets were finally powdered and triturated well. A quantity of powder equivalent to 10 mg of drug were transferred to 10 ml volumetric flask, and 8 ml of mobile phase was added and solution was sonicated for 15 minutes, there after volume was made up to 10 ml with same solvent. Then 1ml of the above solution was diluted to 10 ml with HPLC grade methanol. The solution was filtered through a membrane filter (0.45 μm) and

sonicated to degas. From this stock solution (1.0 ml) was transferred to five different 10 ml volumetric flasks and volume was made up to 10 ml with same solvent system²⁸⁻²⁹.

The solution prepared was injected in five replicates into the HPLC system and the observations were recorded.

A duplicate injection of the standard solution was also injected into the HPLC system and the peak areas were recorded. The data are shown in Table-12.

ASSAY

$$\text{Assay} = \frac{\text{AT}}{\text{AS}} \times \frac{\text{WS}}{\text{DS}} \times \frac{\text{DT}}{\text{WT}} \times \frac{\text{P}}{100} \times \frac{\text{AW}}{\text{LC}} \times 100$$

Where:

AT = Peak Area of Etelcalcetide obtained with test preparation

AS = Peak Area of Etelcalcetide obtained with standard preparation

WS = Weight of working standard taken in mg

WT = Weight of sample taken in mg

DS = Dilution of Standard solution

DT = Dilution of sample solution

P = Percentage purity of working standard

Results obtained are tabulated below³⁰:

Table-12: Assay of Etelcalcetide in Pharmaceutical Dosage Forms

Brand name of Tablets/Capsules	Labelled Amount of Drug (mg)	Mean ($\pm$ SD) Amount (mg) Found by the Proposed Method (n=5)	Assay + % RSD
Parsabiv Injection (Amgen)	10mg/2ml	9.564 ($\pm$ 0.384)	99.457 % ($\pm$ 0.387)

Result & Discussion: The %Purity of Parsabiv Injection containing Etelcalcetide was found to be 99.475% ($\pm$ 0.387).

SUMMARY AND CONCLUSION:

The analytical method was developed by studying different parameters. First of all, maximum absorbance was found to be at 245nm and the peak purity was excellent. Injection volume was selected to be 10 μ l which gave a good peak area. The column used for study was Symmetry C18, 250 mm x 4.6 mm i.d. 5 μ m particle size because it was giving good peak. Ambient temperature was found to be suitable for the nature of drug solution. The flow rate was fixed at 1.0ml/min because of good peak area and satisfactory retention time. Mobile phase is Methanol: Phosphate Buffer (0.02M) (pH-3.8) (70: 30% v/v) was fixed due to good symmetrical peak. So this mobile phase was used for the proposed study. Methanol was selected because of maximum extraction sonication time was fixed to be 10min at which all the drug particles were completely soluble and showed good recovery. Run time was selected to be 7min because analyze gave peak around 2.775min and also to reduce the total run time. The percent recovery was found to be 98.0-102 was linear and precise over the same range. Both system and method precision was found to be accurate and well within range. The analytical method was found linearity over the range of 6-14ppm of the Etelcalcetide target concentration. The analytical passed both robustness and ruggedness tests. On both cases, relative standard deviation was well satisfactory.

BIBLIOGRAPHY:

- <https://go.drugbank.com/drugs/DB12865>
- <https://pubchem.ncbi.nlm.nih.gov/compound/Etelcalcetide>
- <https://en.wikipedia.org/wiki/Etelcalcetide>
- R. Snyder, J. Kirkland, L. Glajch, Practical HPLC Method Development, John Wiley and Sons International publication, II Edn., 2011.
- S. Ashutoshkar, Pharmaceutical Drug Analysis 2nd Edn, New Age International Private Limited Publishers, 452-474, 2005.
- H. Beckett and J.B. Stenlake, Practical Pharmaceutical Chemistry, 4th Edn. C.B.S. Publishers and Distributors, New Delhi. 1-9, 157-167.
- H.H. Williard, L.L. Merit, F.A. Dean, F.A. Settle, Instrumental Methods Of Analysis, 6th Edn, C.B.S. Publishers and Distributors, New Delhi.: 430-440, 495-504, 529-545.
- B.K. Sharma, Instrumental Methods of Chemical Analysis. GOEL Publishing House, Meerut: 286-300.
- Instant notes on analytical chemistry by D. Kealey and P.J. Haines, © BIOS Scientific Publishers Limited, UK, 6-7, 2002.
- Gurdeep R. Chatwal, Sham K. Anand, Instrumental methods of Chemical Analysis, 5th edition, Himalaya Publishing House (Mumbai), P-2.566, 2005,.
- M. E. Swartz, Journal of liquid chromatography, 28(7/8), 1253-1263(2005).
- Journal of Chromatography .B, Analytical Technologies in the Biomedical and life Sciences. 2008 March 1; 863(2): 258-265. Published on Jan 18 2008.
- International Conference on Harmonization, Harmonized Tripartite Guideline. Validation of Analytical Procedures. Text and Methodology. Q2 (R1). November 2005.
- International Conference on Harmonization (ICH). Validation of Analytical Methods: Definitions and Terminology. ICH Q2A. 1994.
- J. M. Green, a practical guide to analytical method validation, anal. Chem. News & features, pp. 305a-309a, 1 may 1996.
- P. A. Winslow and r. F. Meyer, defining a master plan for the validation of analytical methods, j. Validation technology, pp. 361-367, 1997.
- Aoac peer-verified methods program, manual on policies and procedures, Arlington, Va., USA (1998).
- R. Patil: J of Chromatographia, 67, 575, (2008).
- Baht and Leena: J of Liq. Chrom., 30, 309, (2007).
- H.H. Williard, L.L. Merit, F.A. Dean and F.A. Settle, Instrumental methods of analysis, 7th edition, C.B.S. Publishers, New Delhi, 2002.
- GN Menon, LB White, Department of Analytical Research, Abbott Laboratories, (pub med-index for MEDLINE).
- Food and Drug Administration (FDA), "Analytical Procedures and Methods Validation: Chemistry, Manufacturing and Controls Documentation;" Federal Register (Notices), Vol: 65 (169), 52776-52777, 2000.
- Vibha G et al., Development and validation of HPLC method - a review. International

- Research Journal of Pharmaceutical and Applied Sciences. 2012, 2(4), 22-23.
24. Bliesner DM. In: Validating Chromatographic Methods. John Wiley & sons Inc. 2006, 88-92.
 25. Validation of Analytical Procedures: Methodology. ICH-Guidelines Q2B, Geneva. 1996, 11. (CPMP/ICH/281/95).
 26. Development and validation of HPLC method - A Review, Vibha Gupta et al, International Research Journal of Pharmaceutical and Applied Sciences, 2012; 2(4):17-25.
 27. A Review: HPLC Method Development and Validation, Santosh Kumar Bhardwaj *et al. International Journal of Analytical and Bioanalytical Chemistry, accepted 20 November 2015.
 28. Method Development: A Guide to Basics Quantitative & Qualitative HPLC, LC, GC ChromAcademy.
 29. Lalit V Sonawane* Bioanalytical Method Validation and Its Pharmaceutical Application- A Review Pharmaceutica Analytical Acta 2014, 5:3Center for Drug Evaluation and Research (CDER) Reviewer Guidance.
 30. ICH Topic Q 2 (R1) Validation of Analytical Procedures: Text and Methodology.
 31. Krishna Kishore Adireddy*, Srinivasa Rao Baratam, Nagarjuna Hari Pratap S., RP-HPLC Method for Quantification of Etelcalcetide in Bulk and Parenteral Dosage Form, Research Journal of Pharmacy and Technology, 2021; 14(10):5521-6, Doi: 10.52711/0974-360X.2021.00963.
 32. Shabana Sultana1*, Dr R. Vani 2, Dr M. Sunitha3, Analytical Method Development and Validation for the Estimation of Etelcalcetide in Bulk and its Dosage Form Using RP-HPLC, Indo American Journal of Pharmaceutical Research, 2017, Vol 7, Issue 11, Pages: 928-934.
 33. Sivaji Maganti1,2, Suryakala Duvvuri1,* Srivathsa Degekar Gouni2,3, Pavani Kadupu2, And M. Bhaskara Praveen Varma2, RP-HPLC Method for the Quantification of Impurities in Etelcalcetide Injection and a Comparative Characterization Study of In-House Samples of Etelcalcetide Injection with Reference-Listed Drug Samples, Asian Journal of Chemistry; Vol. 37, No. 4 (2025), 968-974.